

# A Guide to Inogen Rove 6 Portable Oxygen Machine



# Contents

Portable Oxygen Machines **3**

Getting to Know the Parts of Your Inogen **4**

How to use your Inogen Rove 6 **5**

Typical New Battery Pack Operation Time **6**

Be Safe **7**

Troubleshooting **8**



**ENHANCING  
LIVES**



## Portable Oxygen Machines

A portable oxygen machine is a small device that can allow you to move around outside and inside of your home. The machine can run using electricity, battery or plugged into the DC outlet in a vehicle.

**It is important that the flow setting requested by your Healthcare Professional is used.**

Please note: Your Inogen Rove 6 remains the property of Baywater Healthcare and is on loan to the NHS

# Getting to Know the Parts of Your Inogen




- A** Nasal prong fitting
- B** Control panel (top)
- C** Exhaust vent
- D** Battery pack
- E** Air inlet
- F** USB port - for service only (behind filter)

## Caution

Ensure the oxygen machine is kept upright at all times.

Make sure the flow setting on the oxygen machine is set to the flow setting ordered by your Healthcare Professional.

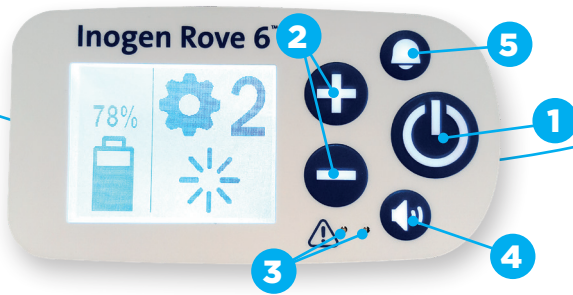

# How to use your Inogen Rove 6



## 1. On/Off button

Press once to turn on, press and hold for one second to turn off. Press briefly for backlight.



## 2. Increase or decrease flow setting button

Use these buttons to set the flow to your prescribed level.



## 3. Indicator lights

Please call Baywater Healthcare if you observe a red or amber light.



## 4. Volume control button

Pressing this button will change the volume level from 1 to 4.



## 5. Audible alert button

Pressing the button will turn an alarm on/off that can detect each time you take a breath. The machine will alarm and will start to release oxygen intermittently if you do not take a breath for more than 60 seconds when the audible alert button is highlighted on the screen.

(open 24 hours, 7 days a week for urgent calls)

# Typical New Battery Pack Operation Time

The following table shows the typical time a new battery pack will last using the various flow settings.

| Flow rate setting | Standard battery duration |
|-------------------|---------------------------|
| 1                 | 12 hours 45 mins          |
| 2                 | 10 hours 15 mins          |
| 3                 | 6 hours 30 min            |
| 4                 | 5 hours 15 mins           |
| 5                 | 3 hours 30 mins           |
| 6                 | 2 hours 30 mins           |

## Battery indication chart

|                   |   |
|-------------------|---|
| 4 LEDs lit        | 75% to 100% full  |
| 3 LEDs lit        | 50% to 75% full   |
| 2 LEDs lit        | 25% to 50% full   |
| 1 LEDs lit        | 10% to 25% full   |
| 1 LEDs (blinking) | Battery is less than 10% full and needs to be recharged |

## Caution

Keep your battery pack dry at all times. If it becomes exposed to liquid stop using immediately and call Baywater Healthcare. Wet battery packs can present safety hazards including fire and electric shock.

# Be Safe

- Keep the Inogen and the power cord away from hot surfaces and flames.
- Do not use if it has a damaged power cord or plug.
- Your Inogen should be used in a place with good air flow around it.
- Only use this device with accessories specified by us.
- If the Inogen has been dropped, damaged or exposed to water, please stop using it and call Baywater Healthcare on **0800 373580**.
- Do not block the air inlet or the exhaust vent of the Inogen.
- Do not cover the device with a blanket, towel or quilt etc.
- When using in a vehicle, be sure it is properly secured in an upright position, belted or otherwise restrained.
- Do not leave your Inogen, or battery pack, in the seating area or boot of your motor vehicle during a hot or very cold day.

## Caution

Do not wrap the power cord around the power pack.

Ensure you only use the Inogen Rove 6 power cord.

Do not leave equipment on show when your vehicle is unattended.

Always remove batteries from the Inogen Rove 6 when not in use.

Do not plug the Inogen Rove 6 into faulty wall sockets and wherever possible unplug it when it is not in use.

# Troubleshooting

## What to do if no oxygen is being produced

No oxygen indicates that the device may be turned off, try pressing the power button to turn on and check battery charge. Check nasal prongs are connected correctly, if none of these checks work, please call Baywater Healthcare on **0800 373580**.

## What to do if the portable oxygen machine does not turn on when the on button is pressed

Portable oxygen machine does not power on when the on button is pressed. First check the battery pack is connected properly. If the battery pack is already connected properly, it may have not enough charge to turn the device on, plug the device into electricity mains to charge. If these checks do not work, please call Baywater Healthcare on **0800 373580**.



## What to do if the no breath detected alarm continues to sound, or no hissing can be heard when breathing

No breath detected alarm continues to sound, or no hissing can be heard when breathing. Please contact your Healthcare Professional as you may require a clinical review.

**If the steps above do not fix the problem, please call Baywater Healthcare for further guidance.**











For more information please contact:

**Baywater Healthcare**

Wulvern House  
Electra Way  
Crewe  
Cheshire  
CW1 6GW


Call:0800 373580

 [healthuk@baywater.co.uk](mailto:healthuk@baywater.co.uk)

 @BaywaterHealth

 Baywater Healthcare

 Baywater Healthcare



Mae'r daflen hon ar Gael yn Gymraeg

**ENHANCING  
LIVES**

23/664/UK-AUG23 v1